


## **1J1002 4 to 2 BNC Converter**

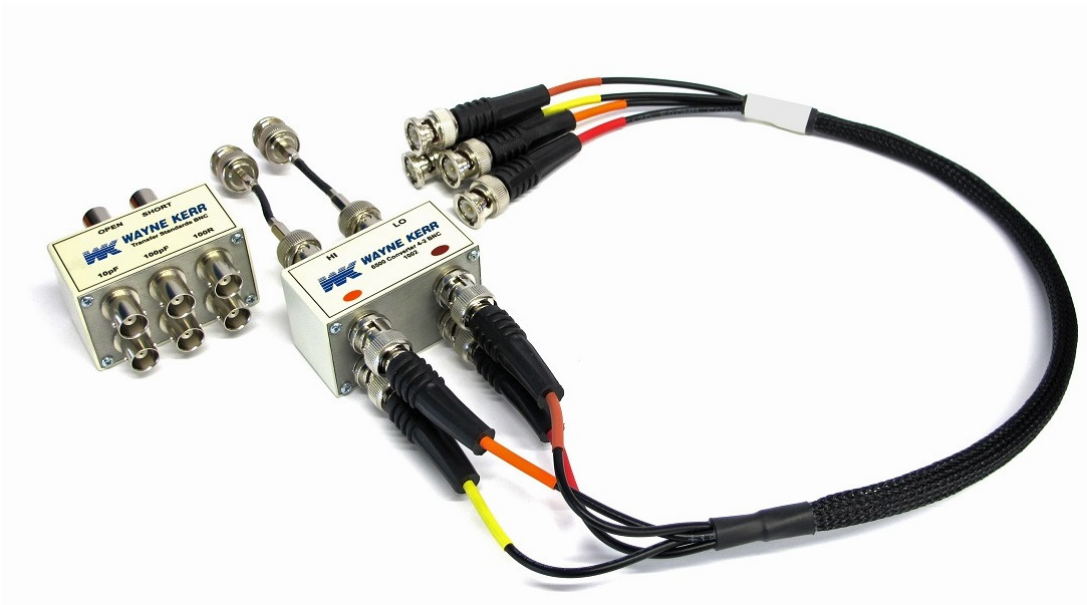

The 1J1001 4 to 1 BNC Converter is used to connect a Wayne Kerr 6500 analyzer to the Device Under Test which is terminated in two BNC connectors.

The outers of the two BNC's should be joined together at the DUT.

### **Suitable models**

6500B series Precision Impedance Analyzer  
6500P series HF LCR Meter

### **Specification**

Frequency:	20 Hz to 120 MHz
Connection to Analyzer:	4-BNC 1 metre cable
Connection to DUT:	Two 8cm coaxial cables, each terminated with a male BNC
Transfer Standards:	5-654-7014 Transfer Standard Box (supplied as standard) Containing Open, Short, 10 pF, 100 pF, 100Ω standards

### **UK GLOBAL HQ**

Wayne Kerr Electronics Ltd. Unit 1A, Durban Road, Bognor Regis, West Sussex, PO22 9QT

**[www.waynekerrtest.com](http://www.waynekerrtest.com)**

Issue D